Equashield Closed System Transfer Device (CSTD) Supplies

Leur Lock Adaptor:	Female Connector:	Protective Plug:
Purpose: connects to end cap of your IV	Purpose: connects to syringe and end of tubing	Purpose: protects the end of female connector from contamination

Medication delivery with CSTD

Medication ball with CSTD	Changes: 1. Female connector placed at the end of the tubing 2. New spike connector	CADD Solis Administration Bag with CSTD

FAIRVIEW

Ganciclovir - Connecting

1. Gather Supplies:
   a) Hand foam
   b) Alcohol wipes
   c) One (1) syringe of saline solution (0.9% sodium chloride)
   d) One (1) leur lock adaptor
   e) New medication with female connector already attached

***Gloves are not needed**

2. Wash your hands for 15 seconds with liquid soap and water or hand foam.

3. Use new alcohol wipe to scrub the end cap on your IV line. Scrub for 15 seconds and let air-dry.

4. Take cap off the saline syringe, and twist syringe into the end cap of line. “Pulse” flush with saline

5. Set up supplies. Open leur lock adaptor package without touching the end.

6. Use new alcohol wipe to scrub the end cap on your IV line. Scrub for 15 seconds and let air-dry.

Ganciclovir - Connecting

7. Twist on leur lock adaptor to the end cap on your IV line.

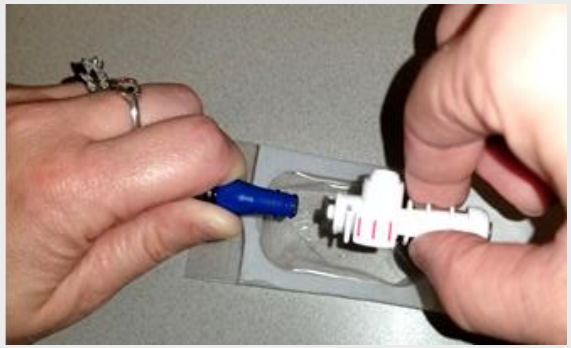

8. Use new alcohol wipe to scrub the end of the leur lock adaptor. Scrub for 15 seconds and let air-dry

9. Remove red protective plug on the end of the medication tubing. *Be careful not to touch leur lock adaptor*

10. Line up red to red, and push-on female connector to leur lock adaptor until you hear a click

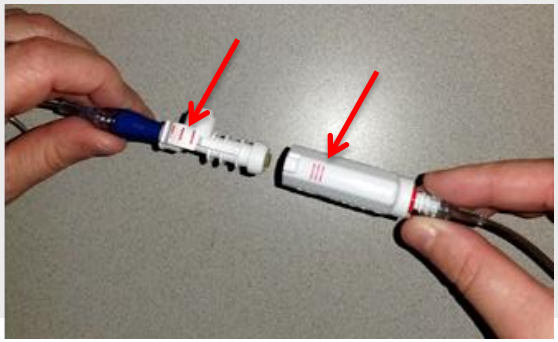

11. To begin infusion, refer to education on CADD or IV Medicine Ball

Please call Fairview Home Infusion if you have any questions

(612)-672-2233

Ganciclovir - Disconnecting

1. Gather Supplies:
   a) Hand foam
   b) Alcohol wipes
   c) One (1) syringe of saline solution (0.9% sodium chloride)
   d) One (1) female connector
   e) Heparin, if needed

   ***Gloves are not needed**

2. Wash your hands for 15 seconds with liquid soap and water or hand foam.

3. Set up supplies and attach female connector to prefilled syringe

4. Disconnect medication by pressing down on red lever and pulling apart.

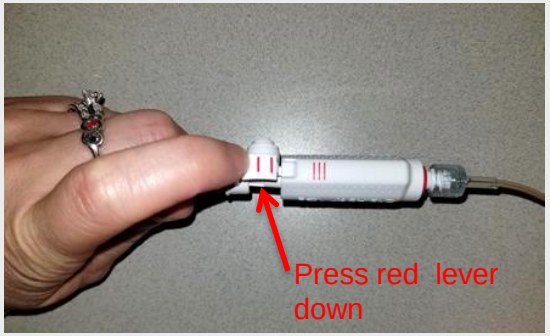

5. Use new alcohol wipe to scrub the end of the leur lock adaptor. Scrub for 15 seconds and let air-dry

6. Remove red protective cap on the end of saline flush. Line up red to red, and push-on female connector to leur lock adaptor until you hear a click. "Pulse" flush your IV line.

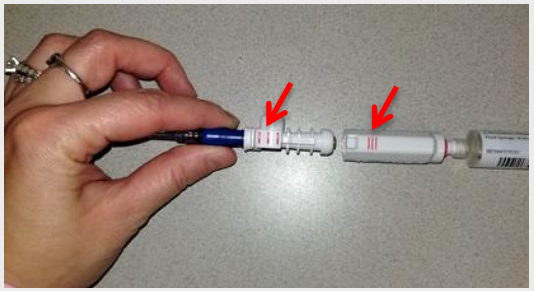

FAIRVIEW

Ganciclovir - Disconnecting

7. Disconnect saline syringe by pressing on red lever and pulling apart.

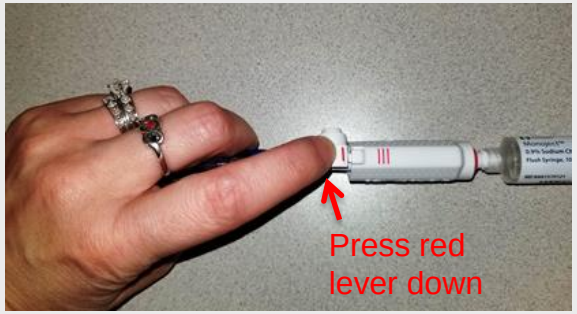

8. Twist off leur lock adaptor from your IV end cap.

9. If heparin is ordered –
Use a fresh alcohol wipe to scrub the end cap on your IV line. Scrub for 15 seconds and let air-dry.

10. Twist on the syringe of heparin and flush

11. Throw away the used medication, tubing, and supplies that have a CSTD attached in black waste container.

Please call Fairview Home Infusion if you have any questions

(612)-672-2233

FAIRVIEW